CORA Cork Open Research Archive
Cartlann Taighde Oscailte Chorcaí

Title	Theoretical study of combined acousto-optical tomography and slow light filters
Authors	Gunther, Jacqueline;Walther, Andreas;Rippe, Lars;Kröll, Stefan;Andersson-Engels, Stefan
Publication date	2018-04-03
Original Citation	Gunther, J., Walther, A., Rippe, L., Kröll, S. and Andersson-Engels, S. (2018) 'Theoretical Study of Combined Acousto-optical Tomography and Slow Light Filters', OSA Technical Digest. Biophotonics Congress: Biomedical Optics Congress 2018 (Microscopy/Translational/Brain/OTS), Hollywood, Florida, Optics InfoBase Conference Papers, Hollywood, Florida, United States, OF1D.3 (3 pp). doi: 10.1364/OTS.2018.OF1D.3
Type of publication	Conference item
Link to publisher's version	https://www.osapublishing.org/abstract.cfm?URI=OTS-2018-OF1D.3 - 10.1364/OTS.2018.OF1D.3
Rights	© 2018 The Author(s); © OSA 2018
Download date	2026-11-06 22:01:01
Item downloaded from	https://hdl.handle.net/10468/11800


UCC
University College Cork, Ireland
Coláiste na hOllscoile Corcaigh

Theoretical Study of Combined Acousto-optical Tomography and Slow Light Filters

Jacqueline Gunther[a], Andreas Walther[b], Lars Rippe[b], Stefan Kröll[b], Stefan Andersson-Engels[a,c]
[a]*Tyndall National Institute, Lee Maltings, Dyke Parade, Cork, Ireland T12 R5CP*
[b]*Department of Physics, Lund University, 221 00 Lund, Sweden*
[c]*Department of Physics, University College Cork, Cork, Ireland*
jacqueline.gunther@tyndall.ie

Abstract: Monte Carlo simulations were used to determine the contrast-to-noise ratio of acousto-optical tomographic imaging with slow light filters versus possible imaging depth. Both reflection and transmission setups were considered. The theoretical model showed that imaging through 12 cm of breast tissue could be plausible. © 2018 The Author(s)
OCIS codes: (170.0170) Medical optics and biotechnology (170.1065) Acousto-optics; (170.3660) Light propagation in tissues

1. Introduction

Optical imaging of biological tissue has good molecular contrast but poor spatial resolution and penetration depth of near infrared light. Acousto-optical tomography (AOT) has the potential to overcome these current imaging limitations. AOT illuminates light through an ultrasound (US) focus in a medium, where photons become "tagged" [1-3]. The tagged light can then be detected using various methods, such as speckle contrast analysis, heterodyne digital holography, photorefractive crystal interferometry, and spectral hole burning methods [1, 2].

We recently published a review of AOT methods [1]. The field has begun roughly the same time as a photoacoustic tomographic (PAT) imaging, but has not gained the same traction and has remained mostly in phantom imaging stage. We identified several challenges that the field still faces to push AOT into in vivo imaging. For example, the decorrelation time of tissue is <1 ms and imaging must take place within this time limit. Also, there needs to be imaging within the tissue optical window, most studies in the review used between 532-638 nm or >1000 nm lasers for imaging [1]. However, despite these challenges, we believe that AOT holds the potential for deep tissue optical imaging. One group used photorefractive crystals and two-wave mixing to image through a 9.4 cm tissue phantom [4]. Another study imaged through a 9 cm tissue phantom, by using slow light filters (SLFs) [5]. Continuing with the concept of combined AOT and SLFs, a theoretical study showed that the imaging depth of AOT could be twice that of PAT in a reflection setup [3]. The study was expanded to use Monte Carlo (MC) simulations instead of the 1D diffusion approximation with boundary conditions and looked at both reflection and transmission geometries. The theoretical study found that imaging through a ~12 cm slab of tissue may be possible with SLFs [6].

SLFs are created by using rare earth crystals and spectral hole burning methods. By pumping the rare earth crystal with a particular laser frequency (i.e. the tagged light frequency) the crystal becomes "transparent" to that frequency of light and absorbs other frequencies. By combining slow light effects, the tagged light also travels slower through the crystal (~μs slower) and aids in the separating the tagged and untagged light [5]. In the previously mentioned SLF study, the untagged light suppression was 30 dB [5]. However, advancements have been made and now the SLFs have a background light suppression of 60 dB, but still have not be utilized in AOT applications yet [7].

We have continued to investigate theoretically the ability to combine spectral hole burning (SHB) into an AOT systems using MC simulations. The MC simulations were used to estimate how many photons would travel through a US focus and to a detector. The number of photons are compared with the number of photons from a typical reflection measurement. Therefore, we calculated the contrast-to-noise ratio (CNR) for both reflectance and transmittance configurations to better understand how much contrast can be achieved deep within biological medium. For this study, we concentrate on simulations that would imitate breast imaging.

2. Methods

Previously, we looked at imaging through muscle to obtain measurements on the heart [6]. Here, we examine breast tissue and the ability to distinguish between a localized increase in absorption coefficient (50% increase from background μ_a) and the background absorption. The source was assumed to be an 880 nm pulsed laser. There were

two possible experimental setups taken into consideration: reflectance and transmittance (see Fig. 1). In the reflection setup the laser, US transducer, and detector are on the same side of the medium and the US focus is translated within the medium. The US transducer is placed halfway between the laser and detector. For the transmittance setup, the laser and detector are on opposite sides of a medium of a given length (L). The US transducer is moved laterally and the US focus is moved z_{US} distance from the laser source.

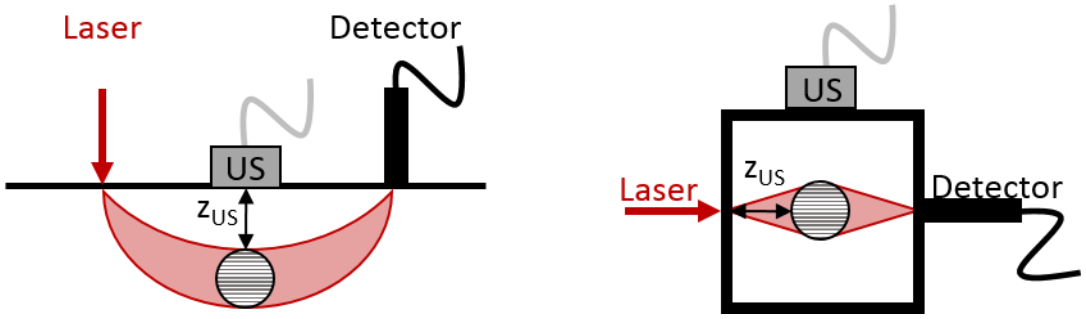


Figure 1 Reflection (Left) and transmission (Right) setups for AOT/SLF simulations. The circle represents the ultrasound focus. US: ultrasound

Monte Carlo simulations were run using parallel computational code that uses the GPU of the computer to effectively decrease computation time [8]. The simulation parameters can be seen in Table 1. The theoretical model is described in reference [6]. Briefly, the fluence map, diffuse reflectance, and diffuse transmittance measurements from the MC simulations are used to determine the number of photons that travel from the source to detector, but also pass through the ultrasound focus (P_{sig}). To obtain the CNR, two signals were calculated: with and without an increase in absorption of the background medium, P_{sig1} and P_{sig2}, respectively. The CNR was calculated using:

$$CNR = \frac{|P_{sig2} - P_{sig1}|}{\sqrt{P_{sig1} + P_{bkg}}} \quad (1)$$

where P_{bkg} are all the untagged photons that were detected.

Table 1 Monte Carlo simulation parameters

Monte Carlo Parameters	**Breast@880 nm[9]**
Photon packages in MC	10^{12}
Absorption coefficient	0.08 cm^{-1}
Scattering coefficient	100 cm^{-1}
Transport scattering coefficient	10 cm^{-1}
Anisotropic factor	0.9
Index of refraction	1.37

3. Results

The CNR for the reflectance setup (Fig. 2 Left) decreases as imaging depth increases. The CNR remains above 1 for to about 6 cm when the source-detector (SD) distance was 2 cm and 4 cm. As for the simulation with SD distance of 6 cm, CNR remains above 1 until about 5.7 cm.

For transmittance, as the length of the medium increased, the CNR decreased. Furthermore, the upper limit for the 10 cm slab had a CNR>10 at every imaging depth. Last, there was a CNR >1 for all depths of the 12 cm slab medium. This simulations showed that 12 cm imaging may be possible if sufficient absorption contrast is attained.

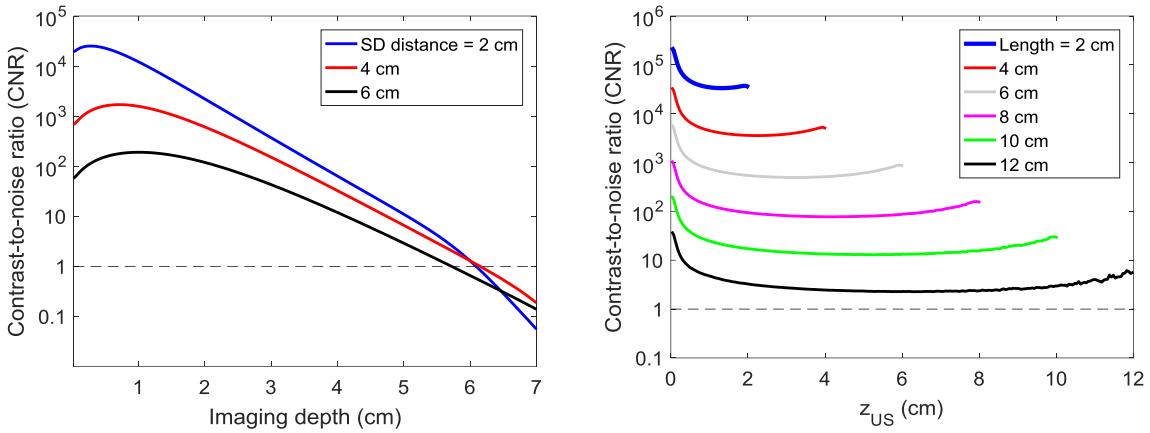


Figure 2 The CNR for reflection (Left) and transmission (Right) setups. The reflection setup shows the CNR for three different source-detector (SD) distances in which the imaging depth is the location of the ultrasound focus in the medium. The transmission setup shows the CNR for different depths of the ultrasound focus (z_{US}) at different lengths of the medium (i.e. 2 cm, 4 cm, etc.). The dash line represents where CNR = 1.

4. Discussion

The general trends of our results are very similar to what was previously observed [3, 6]. However, AOT has shown to image at deeper depths than through muscle [6]. In the current study, a maximum imaging depth with a CNR=1 for reflection geometry was 6 cm. Even with the shorter source-detector distances, the deeper imaging depths were still able to have sufficient contrast to distinguish the two absorptions. The smaller SD distances were more efficient near the boundary of the medium but as the imaging depth increase there was less of a difference in CNR among the different SD distances. Yet, AOT is specific in the sense that if the photon is tagged, then one of the locations of the photon within the medium is known. More investigation is necessary to understand optimal SD distances for reflection AOT.

Also, a slab of length 12 cm would still have sufficient contrast (CNR>1). The CNR remained relatively constant (except near the boundaries) as the ultrasound focus depth was changed, which is unlike the reflection setup. For the reflection setup light not only travels into the medium but then back out again in which case the light path would be a bit more than double the imaging depth. While in the transmission setup, the light travels through the medium [6].

These are promising results that show the possibility of deep tissue imaging when combining spectral hole burning methods with AOT. Yet, phantom studies are still necessary to validate these results.

5. Acknowledgments

This work was supported by the Science Foundation Ireland (SFI/15/RP/2828) and Knut and Alice Wallenberg Foundation (Sweden).

6. References

1. Gunther, J. and S. Andersson-Engels, *Review of current methods of acousto-optical tomography for biomedical applications.* Frontiers of Optoelectronics, 2017.
2. Wang, L.V., *Ultrasound-Mediated Biophotonic Imaging: A Review of Acousto-Optical Tomography and Photo-Acoustic Tomography.* Disease Markers, 2004. **19**(2-3).
3. Walther, A., et al., *Analysis of the potential for non-invasive imaging of oxygenation at heart depth, using ultrasound optical tomography (UOT) or photo-acoustic tomography (PAT).* Biomedical Optics Express, 2017. **8**(10): p. 4523-4536.
4. Lai, P., X. Xu, and L.V. Wang, *Ultrasound-modulated optical tomography at new depth.* Journal of Biomedical Optics, 2012. **17**(6): p. 0660061-0660066.
5. Zhang, H., et al., *Slow light for deep tissue imaging with ultrasound modulation.* Appl Phys Lett, 2012. **100**(13): p. 131102-131102-5.
6. Gunther, J., et al., *Deep tissue imaging with acousto-optical tomography and spectral hole burning with slow light effect: a theoretical study.* (Submitted to JBO), 2017.
7. Kinos, A., et al., *Development and characterization of high suppression and high étendue narrowband spectral filters.* Applied optics, 2016. **55**(36): p. 10442-10448.
8. Alerstam, E., T. Svensson, and S. Andersson-Engels, *Parallel computing with graphics processing units for high-speed Monte Carlo simulation of photon migration.* Journal of Biomedical Optics, 2008. **13**(6): p. 060504-060504-3.
9. Taroni, P., et al., *Breast tissue composition and its dependence on demographic risk factors for breast cancer: non-invasive assessment by time domain diffuse optical spectroscopy.* PloS one, 2015. **10**(6): p. e0128941.