


Title	Accuracy of diagnostic testing in primary ciliary dyskinesia
Authors	Jackson, Claire L.;Behan, Laura;Collins, Samuel A.;Goggin, Patricia M.;Adam, Elizabeth C.;Coles, Janice L.;Evans, Hazel J.;Harris, Amanda;Lackie, Peter;Packham, Samantha;Page, Anton;Thompson, James;Walker, Woolf T.;Kuehni, Claudia;Lucas, Jane S.
Publication date	2016-02-29
Original Citation	Jackson, C. L., Behan, L., Collins, S. A., Goggin, P. M., Adam, E. C., Coles, J. L., Evans, H. J., Harris, A., Lackie, P., Packham, S., Page, A., Thompson, J., Walker, W. T., Kuehni, C. and Lucas, J. S. (2016) 'Accuracy of diagnostic testing in primary ciliary dyskinesia', <i>European Respiratory Journal</i> , 47(3), pp. 837-848. doi: 10.1183/13993003.00749-2015
Type of publication	Article (peer-reviewed)
Link to publisher's version	10.1183/13993003.00749-2015
Rights	© 2016, ERS. ERJ Open articles are open access and distributed under the terms of the Creative Commons Attribution Non-Commercial Licence 4.0. - <a href="https://creativecommons.org/licenses/by-nc/4.0/">https://creativecommons.org/licenses/by-nc/4.0/</a>
Download date	2023-09-28 21:43:49
Item downloaded from	<a href="https://hdl.handle.net/10468/9259">https://hdl.handle.net/10468/9259</a>

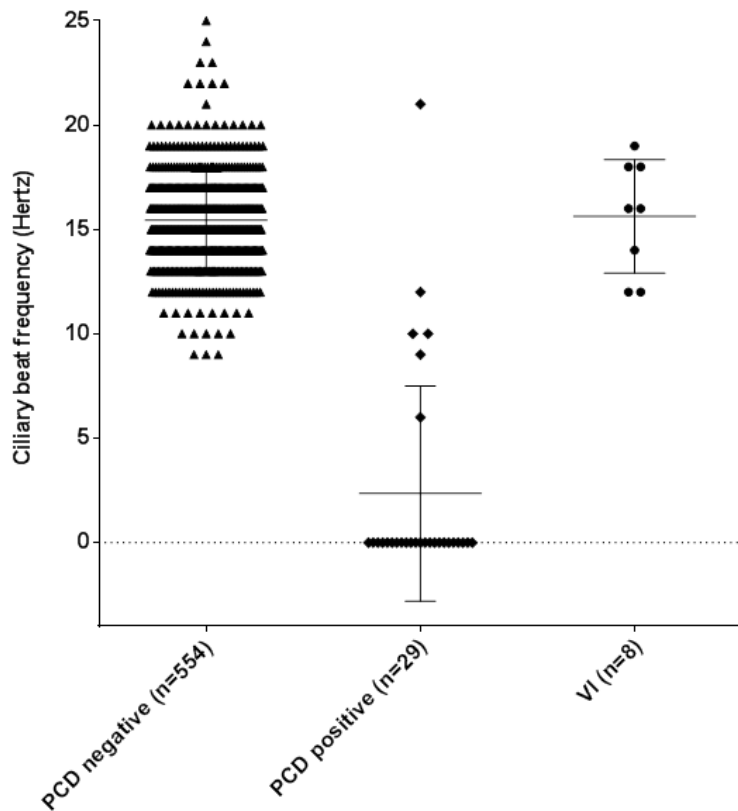

# UCC

**University College Cork, Ireland**  
Coláiste na hOllscoile Corcaigh



**Figure S2:** Individual mean ciliary beat frequency (CBF) values for samples from PCD-negative and PCD-positive and valid-inconclusive (VI) patients. Group mean ( $\pm$ SD): a) nasal brushing biopsies: PCD-negative = 15.4 Hz (2.3), n=554; PCD-positive = 2.3 Hz (5.2), n=29; and VI = 15.6 Hz (2.7), n=8; and b) following air-liquid interface (ALI) culture; PCD-negative = 14.1 Hz (2.3), n=116; PCD-positive = 2.4 Hz (4.2), n=19; and VI = 11.7 Hz (6.3), n=6. One way ANOVA,  $p < 0.0001$ .